


Amp. and Phase vs. time for each freq., 23 segs, 24 APs / seg (12.29 sec / seg.), time ticks 10 sec

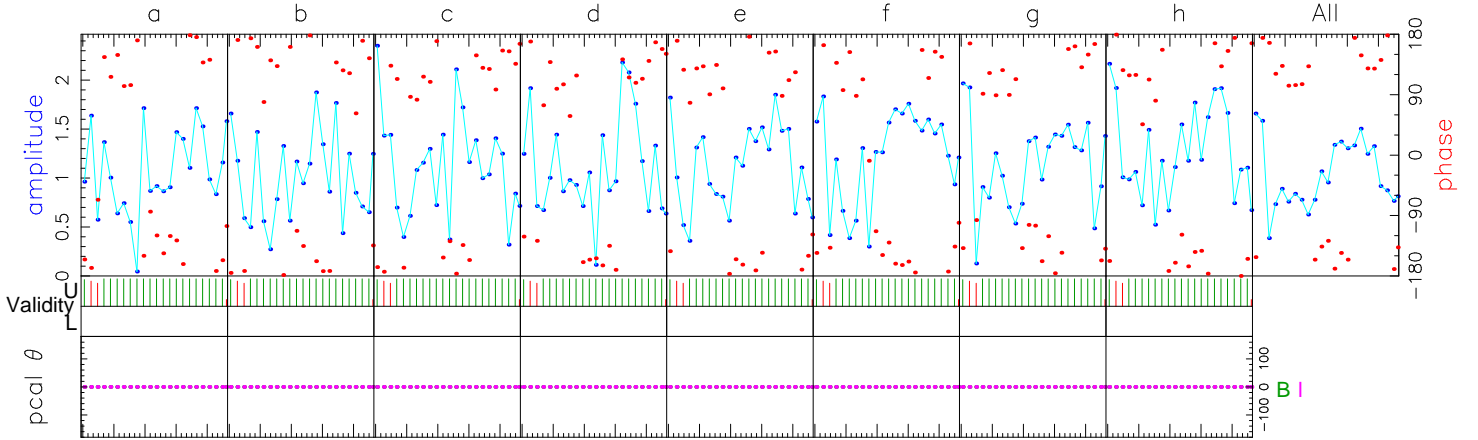

	86124.00	86156.00	86188.00	86220.00	86252.00	86284.00	86316.00	86348.00	Freq (MHz)	All
	-171.7	170.4	157.8	147.9	159.5	178.9	178.0	172.6	Phase	169.2
	0.8	0.8	0.8	0.8	0.8	0.7	0.7	1.0	Ampl.	0.8
	123.3	123.4	123.8	123.5	123.7	123.9	123.6	123.6	Sbd box	123.6
U/L	530/0	530/0	530/0	530/0	530/0	530/0	530/0	530/0	APs used	
B	1000	1000	1000	1000	1000	1000	1000	1000	PC freqs	
I	1000	1000	1000	1000	1000	1000	1000	1000	PC freqs	
B:I	0:0	0:0	0:0	0:0	0:0	0:0	0:0	0:0	PC phase	
B:I	0:0	0:0	0:0	0:0	0:0	0:0	0:0	0:0	ManI PC	
B	1000	1000	1000	1000	1000	1000	1000	1000	PC amp	
I	1000	1000	1000	1000	1000	1000	1000	1000		
B	W00UR	W01UR	W02UR	W03UR	W04UR	W05UR	W06UR	W07UR	Chan ids	
I	W00UR	W01UR	W02UR	W03UR	W04UR	W05UR	W06UR	W07UR	Tracks	
									Chan ids	
									Tracks	
Group delay (usec)(sbd)	-1.11388383929E+04		Apriori delay (usec)		-1.11387816789E+04		Resid mbdelay (usec)		5.78594E-03	+/- 8.3E-05
Sband delay (usec)	-1.11388234864E+04		Apriori clock (usec)		2.2167095E+01		Resid sbdelay (usec)		-4.18075E-02	+/- 6.6E-04
Phase delay (usec)	-1.11387816734E+04		Apriori clockrate (us/s)		3.4699999E-08		Resid phdelay (usec)		5.45587E-06	+/- 1.4E-07
Delay rate (us/s)	-1.57034183781E+00		Apriori rate (us/s)		-1.57034185852E+00		Resid rate (us/s)		2.07048E-08	+/- 9.0E-10
Total phase (deg)			Apriori accel (us/s/s)		6.52598886063E-05		Resid phase (deg)		-190.8	+/- 4.4

	RMS	Theor.	Amplitude	0.823 +/- 0.031	Pcal mode: MANUAL, MANUAL	PC period (AP's) 5, 5	sb window (us)	-1.000	1.000
ph/seg (deg)	41.0	10.5	Search (2048X32)	0.813	Pcal rate: 0.000E+00, 0.000E+00 (us/s)		mb window (us)	-0.016	0.016
amp/seg (%)	48.3	18.3	Interp.	0.000	Bits/sample: 2x2	SampCntNorm: enabled	dr window (ns/s)	-0.011	0.011
ph/frq (deg)	14.3	6.2	Inc. seg. avg.	1.030	Sample rate(MSamp/s): 64		ion window (TEC)	0.00	0.00
amp/frq (%)	9.6	10.8	Inc. frq. avg.	0.829	Data rate(Mb/s): 1024	nlags: 128 t_cohere infinite			

B: az 273.3 el 18.5 pa 41.3 I: az 115.4 el 55.0 pa -49.1 u,v (fr/asec) 9477.886 3028.071 simultaneous interpolator
Control file: cf_1234_gmva Input file: /Exps/c182b/v1/1234/No0239/BI..016HFP Output file: /Exps/c182b/v1/1234/No0239/BI.W.35.016HFP